

# **NREL Spectral Standards Development and Broadband Radiometric Calibrations**

D.R. Myers, A. Andreas, T. Stoffel, I. Reda,  
S. Wilcox, P. Gotseff, and B. Kay  
*National Renewable Energy Laboratory*

C. Gueymard  
*Solar Consulting Services*

*Presented at the National Center for Photovoltaics and  
Solar Program Review Meeting  
Denver, Colorado  
March 24-26, 2003*



**NREL**

**National Renewable Energy Laboratory**

1617 Cole Boulevard  
Golden, Colorado 80401-3393

NREL is a U.S. Department of Energy Laboratory  
Operated by Midwest Research Institute • Battelle • Bechtel

Contract No. DE-AC36-99-GO10337

## NOTICE

The submitted manuscript has been offered by an employee of the Midwest Research Institute (MRI), a contractor of the US Government under Contract No. DE-AC36-99GO10337. Accordingly, the US Government and MRI retain a nonexclusive royalty-free license to publish or reproduce the published form of this contribution, or allow others to do so, for US Government purposes.

This report was prepared as an account of work sponsored by an agency of the United States government. Neither the United States government nor any agency thereof, nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States government or any agency thereof. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States government or any agency thereof.

Available electronically at <http://www.osti.gov/bridge>

Available for a processing fee to U.S. Department of Energy  
and its contractors, in paper, from:

U.S. Department of Energy  
Office of Scientific and Technical Information  
P.O. Box 62  
Oak Ridge, TN 37831-0062  
phone: 865.576.8401  
fax: 865.576.5728  
email: [reports@adonis.osti.gov](mailto:reports@adonis.osti.gov)

Available for sale to the public, in paper, from:

U.S. Department of Commerce  
National Technical Information Service  
5285 Port Royal Road  
Springfield, VA 22161  
phone: 800.553.6847  
fax: 703.605.6900  
email: [orders@ntis.fedworld.gov](mailto:orders@ntis.fedworld.gov)  
online ordering: <http://www.ntis.gov/ordering.htm>



Printed on paper containing at least 50% wastepaper, including 20% postconsumer waste

# NREL Spectral Standards Development and Broadband Radiometric Calibrations


D.R. Myers, A. Andreas, T. Stoffel, I. Reda, S. Wilcox, P. Gotseff, B. Kay  
National Renewable Energy Laboratory, 1617 Cole Blvd, Golden CO 80401  
Dr. Christian Gueymard  
Solar Consulting Services, 174 Bluebird Lane, Bailey, CO

## ABSTRACT

We describe a final version of revisions to current ASTM reference standard spectral distributions used to evaluate photovoltaic device performance. An NREL developed graphical user interface for working with the SMARTS2 spectral model has been developed and is being tested. A proposed ASTM reference Ultraviolet (UV) spectra for materials durability is presented. Improvements in broadband outdoor radiometer calibration, characterization, and reporting software that reduce uncertainties in broadband radiometer calibrations are shown.


## 1. Final Version Revised Spectral Irradiance Standards

We reported on existing and proposed revised consensus standard spectral irradiance distributions at the 2002 IEEE Photovoltaic Specialists Conference [1, 2]. The draft spectra were approved with no negatives by full committee ASTM G03 on weathering and durability. As of January, 2003, the standard will move to full ASTM society-level ballot, probably by June of 2003. If approved with no negative comments the revised standard will be designated as ASTM G173, as the revisions were extensive enough to require a new designation. ASTM G159 will then be withdrawn (as E891 and E892 have been). Figure 1 displays the new air mass 1.5 spectra for hemispherical radiation on a 37° equator-facing tilted surface, and the direct normal plus circumsolar spectrum. The conditions are for sea level air mass (AM) 1.5, rural aerosol profile with optical depth 0.084, United States Standard Atmosphere of 1976, precipitable water 1.42 cm, and ozone of 0.34 atm-cm.

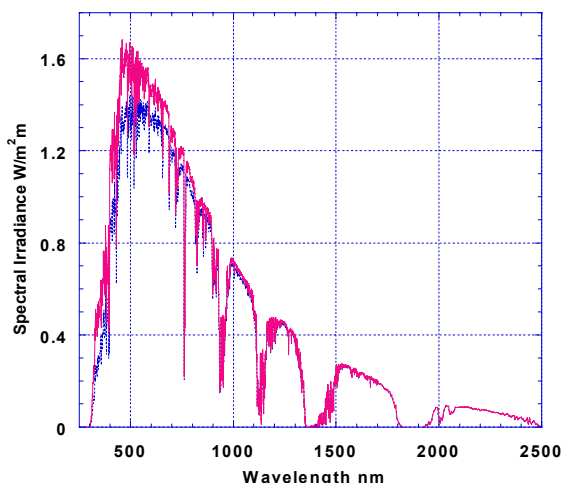

**Figure 1.** Revised direct normal (lower line) and hemispherical 37° tilt spectrum at AM 1.5. Spectra extend to 4000 nm, displayed only to 2500 nm.

The SMARTS2 spectral transmission model [3] is used to compute the revised spectral standards. NREL has developed an Excel®-based user interface to allow users to (1) reproduce the spectra at will, and (2) produce test spectra for different atmospheric conditions for performance comparisons and analysis. Figure 2 shows sample screen shots of the interface.

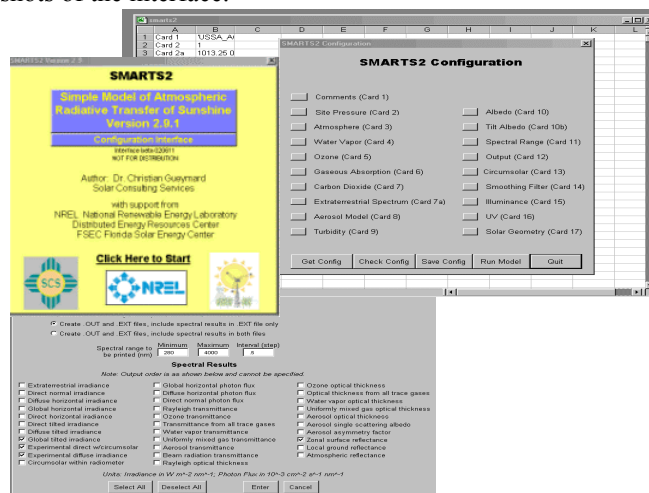


**Figure 2.** NREL-developed Excel Visual Basic based graphical user interface for SMARTS2 model input file configuration.

Later in 2003, after validation testing, we are planning to make the SMARTS2 model and the interface publicly available through the NREL Renewable Resource Data Center (Rredc). Prospective users may contact the lead author at daryl\_myers@nrel.gov to obtain the model, and interface, or more information.

## 2. ASTM Approval of Ultraviolet Reference Standard

During the effort to revise the reference spectra for PV performance applications, the weathering and durability industry participants in ASTM committee GO3 requested the development of a reference Ultraviolet (UV) standard spectrum. Several candidate spectra were proposed, again based on the SMARTS2 spectral model. In Jan. 2003, the committee voted to accept a draft standard proposed by NREL to represent an upper limit for a naturally occurring UV exposure spectrum. The spectrum chosen represents United States Standard Atmosphere (USSA) conditions at air mass 1.05 at 2-kilometer elevation with somewhat reduced total column ozone of 0.30 atm-cm and aerosol optical depth 0.05.


Figure 3 displays the proposed UV reference spectrum, which will be submitted for full ASTM Society ballot later in 2003.

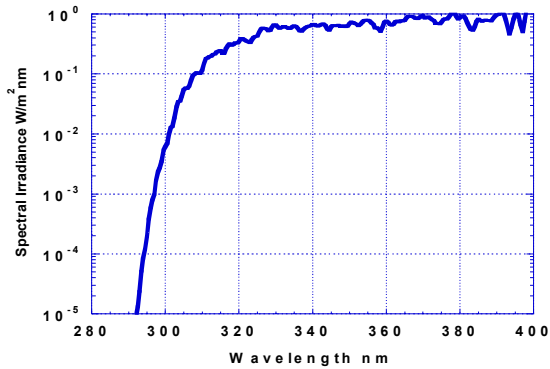

**Figure 3.** Proposed weathering and durability UV reference spectrum for USSA, 2-km Altitude, AM 1.05, Aerosol optical depth of 0.05, and total column O3 of 0.30 atm-cm.

### 3. Broadband Radiometer Calibration Improvements

During 2002, we upgraded our Radiometer Calibration and Characterization (RCC) software for broadband radiometer calibrations at NREL. Improvements include a new graphical user interface, integrated calibration history database, and reporting functionality [4,5]. The new RCC processes responsivity data is based on more accurate diffuse reference irradiance measurements and zenith angle information described in [5] and [6]. The new ISO-compliant calibration report for broadband radiometers is shown in Fig. 4. The new software also performs functional fits to the cosine response curve of each individual radiometer, based on the calibration data in 46 2-degree-wide zenith angle bins.

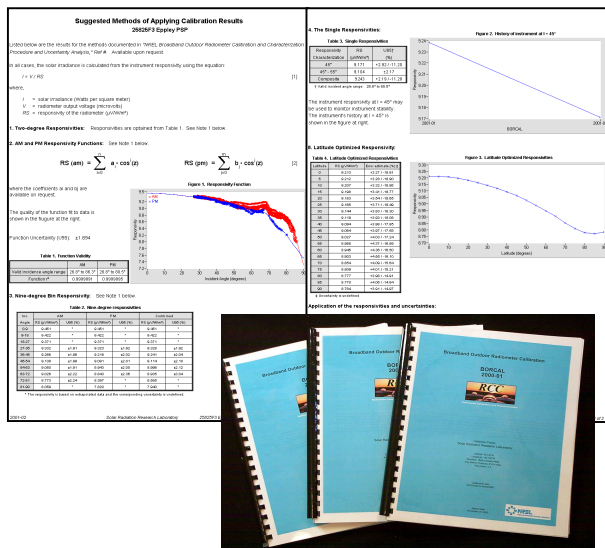


**Figure 4.** Detailed calibration reports as generated by new version of RCC. Hardcopy and CD-rom versions of reports are available to instrument owners.

The form of the fitted function is :

$$Rs(\Theta)_{AM/PM} = \sum_{i=0}^{i=N} a_i \cdot \cos^i(\Theta)$$

where  $\Theta$  is the zenith angle, the  $a_i$  are 46 coefficients (for each of the morning and afternoon zenith angle sets) fit from the calibration data, and  $Rs(\Theta)$  is the responsivity at a given zenith angle. The particular coefficients for fitting the cosine response curve for a given instrument are available upon request at the completion of an NREL BORCAL event. Figure 5 portrays the repeatability of about  $\pm 1\%$  (or 10 W/m<sup>2</sup> at 1000 W/m<sup>2</sup> full scale) of this outdoor determination of cosine response for an NREL control pyranometer over seven BORCAL events in 2001 and 2002.

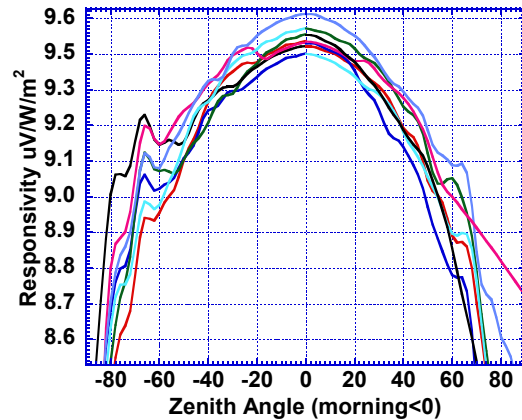

**Figure 5.** Repeatability of control pyranometer fitted cosine response function for seven BORCAL events in 2001/2002.

Variations in the functional fits in Fig. 5 are probably due to changing temperature and solar azimuth geometry over the 2-year period of the calibrations.

### Summary

The Solar Radiometric Measurements task continues to provide technical support for consensus standards, spectral modeling, and optical metrology needs of the PV industry and research and development programs.

### References

1. D. Myers, C. Gueymard, K. Emery. *Proposed Reference Spectral Irradiance Standards to Improve Photovoltaic System Performance Evaluation in 29th IEEE Photovoltaic Specialist Conference*. 2002. New Orleans, LA: Institute of Electrical and Electronic Engineers.
2. D. Myers, C. Gueymard, K. Emery. *Terrestrial Solar Spectral Modeling Tools and Applications for Photovoltaic Devices in 29th IEEE Photovoltaic Specialist Conference*. 2002. New Orleans, LA: Institute of Electrical and Electronic Engineers.
3. C. Gueymard, *Parameterized Transmittance Model for Direct Beam and Circumsolar Spectral Irradiance*. Solar Energy, 2001. **71**(5): p. 325-346.
4. D.R. Myers, T. L. Stoffel, S. Wilcox, I. Reda, A. Andreas, *Recent Progress in Reducing the Uncertainty in and Improving Pyranometer Calibrations*. Journal of Solar Energy Engineering, 2002. **124**: p. 44-50.
5. S.M. Wilcox, *Improved Methods for Broadband Outdoor Radiometer Calibration (BORCAL) in Twelfth Atmospheric Radiation Measurement (ARM) Science Team Meeting, April 8-12, 2002*. 2002. St. Petersburg, Florida: Department of Energy, Atmospheric Radiation Measurement Program.

6. I. Reda., T.L .Stoffel, D. Myers, *A Method to Establish a Clear Sky Diffuse Irradiance Reference For Pyranometer Calibrations*. Solar Energy. **In Press**.

<b>REPORT DOCUMENTATION PAGE</b>			Form Approved OMB NO. 0704-0188	
Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.				
1. AGENCY USE ONLY (Leave blank)	2. REPORT DATE May 2003	3. REPORT TYPE AND DATES COVERED Conference Paper		
4. TITLE AND SUBTITLE NREL Spectral Standards Development and Broadband Radiometric Calibrations		5. FUNDING NUMBERS PVP37401		
6. AUTHOR(S) D.R. Myers, A. Andreas, T. Stoffel, I. Reda, S. Wilcox, P. Gotseff, B. Kay and Dr. C. Gueymard*				
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) National Renewable Energy Laboratory, 1617 Cole Boulevard, Golden, Colorado 80401 *Consultant, 174 Bluebird Lane, Bailey, Colorado 80421-2005		8. PERFORMING ORGANIZATION REPORT NUMBER NREL/CP-560-33468		
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)		10. SPONSORING/MONITORING AGENCY REPORT NUMBER		
11. SUPPLEMENTARY NOTES				
12a. DISTRIBUTION/AVAILABILITY STATEMENT National Technical Information Service U.S. Department of Commerce 5285 Port Royal Road Springfield, VA 22161		12b. DISTRIBUTION CODE		
13. ABSTRACT (Maximum 200 words): We describe a final version of revisions to current ASTM reference standard spectral distributions used to evaluate photovoltaic device performance. An NREL-developed graphical user interface for working with the SMARTS2 spectral model has been developed and is being tested. A proposed ASTM reference Ultraviolet (UV) spectra for materials durability is presented. Improvements in broadband outdoor radiometer calibration, characterization, and reporting software reduce uncertainties in broadband radiometer calibrations.				
14. SUBJECT TERMS: PV; ASTM G173; ASTM standards; BORCAL; PV device performance standard; SMARTS2, UV spectra standard		15. NUMBER OF PAGES		
		16. PRICE CODE		
17. SECURITY CLASSIFICATION OF REPORT Unclassified	18. SECURITY CLASSIFICATION OF THIS PAGE Unclassified	19. SECURITY CLASSIFICATION OF ABSTRACT Unclassified	20. LIMITATION OF ABSTRACT  UL	

NSN 7540-01-280-5500

Standard Form 298 (Rev. 2-89)

Prescribed by ANSI Std. Z39-18  
298-102